



# CERTIFICATE OF ACCREDITATION

## The ANSI National Accreditation Board

Hereby attests that

**Griffin Incorporated**  
**11629 S 700 E**  
**Draper, UT 84020**

Fulfills the requirements of

**ISO/IEC 17025:2017**

In the field of

**CALIBRATION**

This certificate is valid only when accompanied by a current scope of accreditation document.  
The current scope of accreditation can be verified at [www.anab.org](http://www.anab.org).

Jason Stine, Vice President

Expiry Date: 25 February 2027

Certificate Number: AC-3362



This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2017.  
This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory  
quality management system (refer to joint ISO-ILAC-IAF Communiqué dated April 2017).

## SCOPE OF ACCREDITATION TO ISO/IEC 17025:2017

### Griffin Incorporated

11629 S 700 E

Draper, UT 84020

Steven Griffin 801-574-8700 steve@griffinincorporated.com

### CALIBRATION

ISO/IEC 17025 Accreditation Granted: **25 February 2025**

Certificate Number: **AC-3362**

Certificate Expiry Date: **25 February 2027**


#### Length – Dimensional Metrology

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Dial, Digital, Vernier Calipers <sup>1</sup> (Outside, Inside, Step, Depth)	Up to 8 in	410 µin	Comparison to Gage Blocks; ASME B89.1.14, M-01
Outside Micrometers <sup>1</sup> Length Linearity	Up to 6 in	60 µin	Comparison to Gage Blocks; ASME B89.1.13, M-08
Linear Measurements <sup>2</sup>	Up to 10 in	$(28 + 12L) \mu\text{in}$	Measurements made with P&W Model C Supermicrometer®; Internal Procedures

Calibration and Measurement Capability (CMC) is expressed in terms of the measurement parameter, measurement range, expanded uncertainty of measurement and reference standard, method, and/or equipment. The expanded uncertainty of measurement is expressed as the standard uncertainty of the measurement multiplied by a coverage factor of 2 ( $k=2$ ), corresponding to a confidence level of approximately 95%.

#### Notes:

- On-site calibration service is available for this parameter, since on-site conditions are typically more variable than those in the laboratory, larger measurement uncertainties are expected on-site than what is reported on the accredited scope.
- $L$  = length in inches.

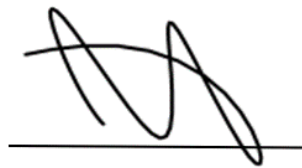

Jason Stine, Vice President